Certificate of Analysis

Polystyrene Standard (30 kDa)

Polystyrene in toluene: dn/dc = 0.110 mL/g; $A_2 = 4.4 \times 10^{-4}$ (mol mL)/g²

Wyatt p/n: 900081
Lot Number: J11430001

Manufactured by: Pressure Chemical Company
Expires: 25 Nov 2028
Storage: Room temperature

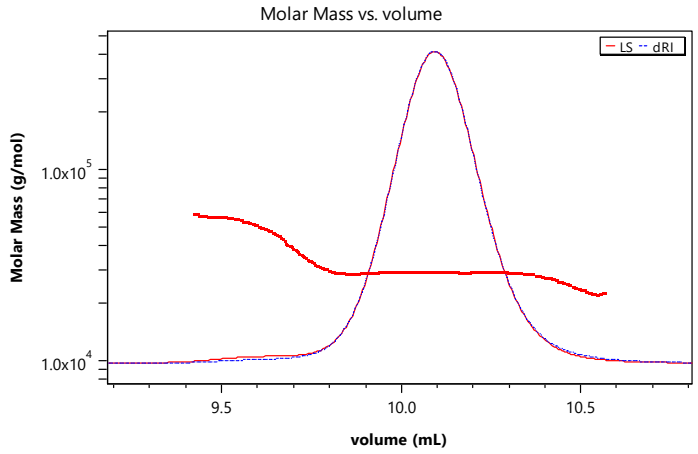

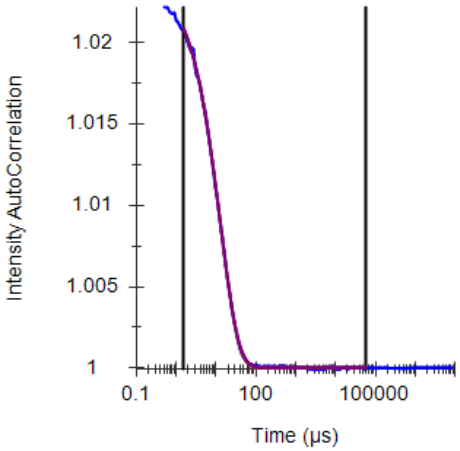

Standard characterization data by Wyatt MALS and ViscoStar™ detectors following SEC separation (MZ-Gel SDplus™ linear 5 µm, 300 mm x 8.0 mm column):

Solvent and SEC mobile phase were toluene. Solution was prepared at 1.67 mg/mL.

Molar Mass (monomer)	M_w = (28.8 ± 0.3) kDa	M_w/M_n = 1.00 ± 0.00
Molar Mass (entire eluted mass)	M_w = (29.2 ± 0.4) kDa	M_w/M_n = 1.01 ± 0.00
Intrinsic Viscosity (monomer)	$[\eta]_w$= (20.4 ± 0.3) mL/g	$[\eta]_z$ = (20.4 ± 0.2) mL/g
Intrinsic Viscosity (entire eluted mass)	$[\eta]_w$= (20.5 ± 0.3) mL/g	$[\eta]_z$ = (20.7 ± 0.4) mL/g

Standard characterization data by Wyatt DynaPro™ NanoStar™ instrument:

Solvent was toluene. Solution was prepared at 1 mg/mL.

R_h (Cumulants) = (4.1 ± 0.1) nm

R_h (Regularization) = (4.5 ± 0.2) nm

Certification: Sophia Kenrick
Sophia Kenrick
Head of Analytical Sciences

Date: 25 Nov 2024

© 2024 Wyatt Technology, LLC. All rights reserved.
One or more of Wyatt Technology's trademarks may appear in this publication. Notably, ViscoStar, DynaPro, and NanoStar are trademarks of Wyatt Technology, LLC. For a list of Wyatt Technology trademarks, please see https://www.waters.com/nextgen/us/en/about-waters/corporate-governance/trademarks.html. All other trademarks are the property of their respective owners.

6330 Hollister Ave, Santa Barbara, CA 93117 USA **T** 805.681.9009 **F** 805.681.0123 waters.com/wyatt