



6330 Hollister Avenue
 Santa Barbara, CA 93117
 Tel. (805) 681-9009
 Fax (805) 681-0123
 email: info@wyatt.com
 www.wyatt.com



Certificate of Analysis

Bovine Serum Albumin (BSA) Ampule

BSA monomer: $M = 66.4$ kDa; $R_h = 3.5$ nm; intrinsic viscosity, $[\eta] = 4.1$ mL/g; $dn/dc = 0.185$ mL/g; extinction coefficient at 280 nm, $\epsilon = 0.667$ mL/(mg cm); $A_2 = 1.0 \times 10^{-4}$ (mol mL)/g² in PBS, pH 7

Wyatt p/n: 900113
 Lot Number: WE326014

Manufactured by: Thermo Scientific®
 Expires: 16 Sep 2022
 Storage: Room temperature

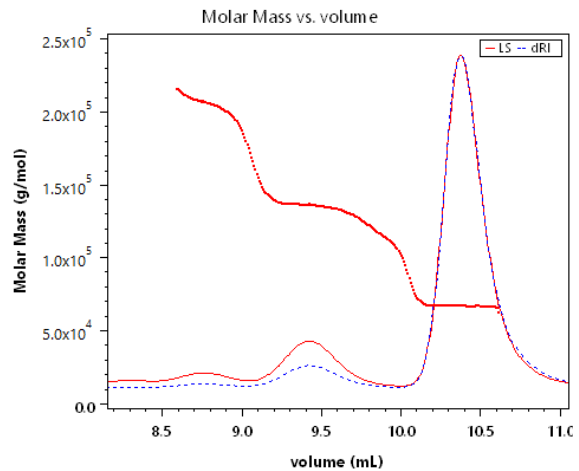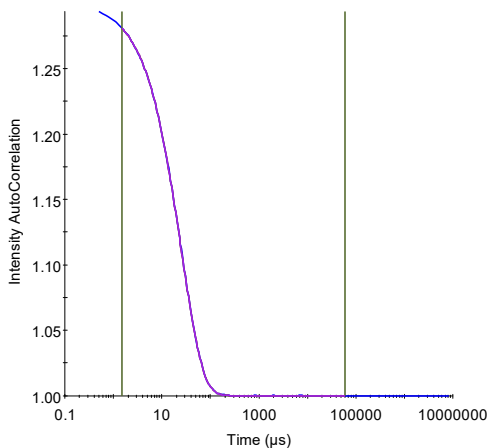

Standard characterization data by Wyatt DynaPro® NanoStar® instrument or Plate Reader:

Solution filtered through 0.02 µm Anotop® filter

R_h (Cumulants) = (3.9 ± 0.1) nm

R_h (Regularization) = (4.2 ± 0.1) nm

Solution filtered through 0.2 µm Anotop filter

R_h (Cumulants) = (4.6 ± 0.1) nm

R_h (Regularization) = (4.1 ± 0.1) nm

Standard characterization data by Wyatt MALS detector following SEC separation (WTC-30S5 with PBS at 0.5 mL/min):

Solution filtered through 0.02 µm Anotop filter

Monomer mass fraction = (88.3 ± 0.1) %

M_w (including aggregates) = (78.1 ± 0.3) kDa

Solution filtered through 0.2 µm Anotop filter

Monomer mass fraction = (88.4 ± 0.6) %

M_w (including aggregates) = (78.9 ± 2.9) kDa

Certification: Sophia Kenrick
 Sophia Kenrick
 Director of Analytical Sciences

Date: 16 Sep 2021