



WYATT
TECHNOLOGY

6330 Hollister Avenue
Santa Barbara, CA 93117
Tel. (805) 681-9009
Fax (805) 681-0123
email: info@wyatt.com
www.wyatt.com



Certificate of Analysis

Batch DLS Size Standard (50 nm nominal radius)

Polystyrene latex spheres suspended in 10 mM sodium phosphate, pH 7.2, at 0.001% w/v
($\sim 2 \times 10^{10}$ particles/mL)

Wyatt p/n: 900175
Lot Number: W050SD0224

Prepared by: Wyatt Technology Corporation
Expires: 31 Aug 2025
Storage: 2-8 °C after opening, DO NOT FREEZE

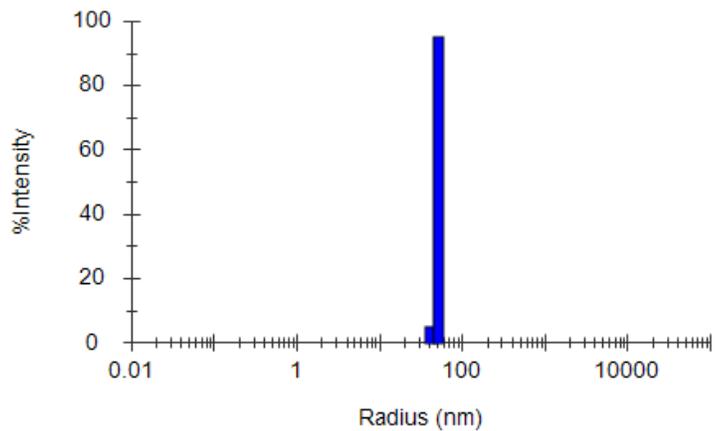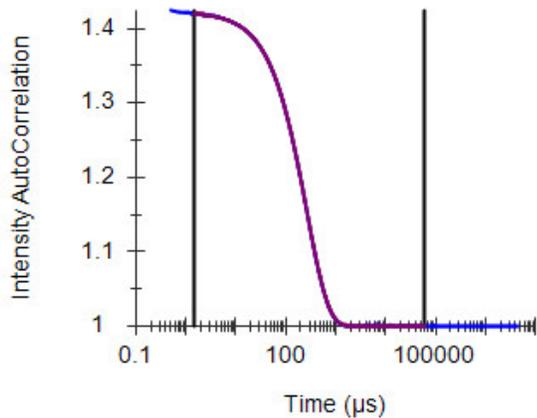

Standard characterization data by Wyatt DynaPro® dynamic light scattering instruments:

Sample was measured neat at 25 °C.

R_h (Cumulants) = (49 ± 1) nm

R_h (Regularization) = (51 ± 1) nm

Certification: Sophia Kenrick
Sophia Kenrick
Head of Analytical Sciences

Date: 27 Aug 2024