





Certificate of Analysis

Batch DLS Size Standard (150 nm nominal radius)

Polystyrene latex spheres suspended in 10 mM sodium phosphate, pH 7.2, at 0.0001% w/v
($\sim 1 \times 10^8$ particles/mL)

Wyatt p/n: 900174
Lot Number: W150SD0224

Prepared by: Wyatt Technology, LLC
Expires: 04 Apr 2026
Storage: 2-8 °C after opening, DO NOT FREEZE

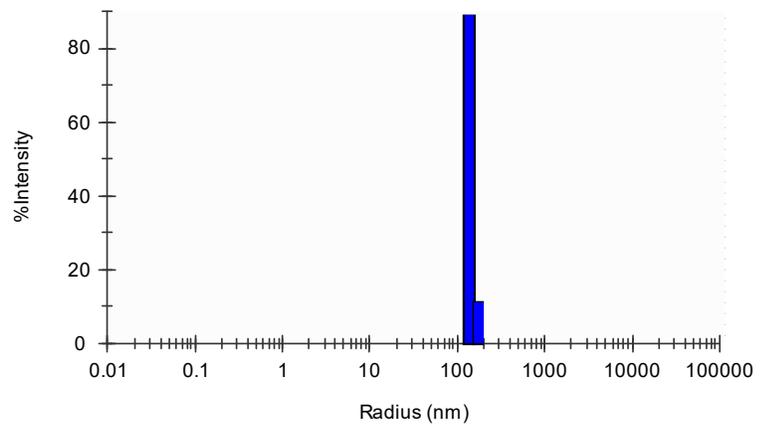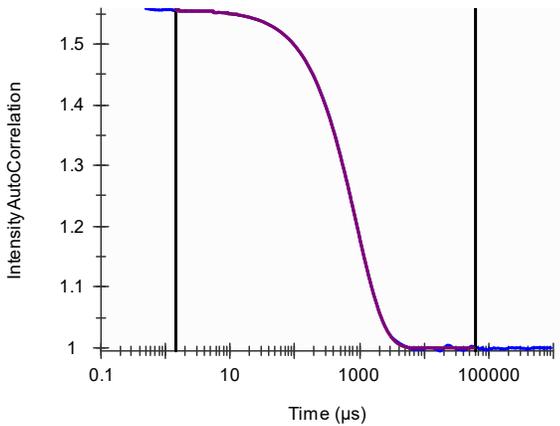


Standard characterization data by Wyatt DynaPro™ dynamic light scattering instruments:

Sample was measured neat at 25 °C with solvent viscosity 0.90 cP.

R_h (Cumulants) = (142 ± 3) nm

R_h (Regularization) = (143 ± 5) nm

Certification: 
Sophia Kenrick
Director, Analytical Sciences

Date: 04 Apr 2025

© 2024 Wyatt Technology, LLC. All rights reserved.
One or more of Wyatt Technology's trademarks may appear in this publication. Notably, DynaPro is a trademark of Wyatt Technology, LLC. For a list of Wyatt Technology trademarks, please see <https://www.waters.com/nextgen/us/en/about-waters/corporate-governance/trademarks.html>. All other trademarks are the property of their respective owners.