



6330 Hollister Avenue
Santa Barbara, CA 93117
Tel. (805) 681-9009
Fax (805) 681-0123
email: info@wyatt.com
www.wyatt.com

Certificate of Analysis

Batch DLS Size Standard (150 nm nominal radius)

Polystyrene latex spheres suspended in 10 mM sodium phosphate, pH 7.2, at 0.0001% w/v
($\sim 1 \times 10^8$ particles/mL)



Wyatt p/n: 900174

Lot Number: W150SD0323A

Prepared by: Wyatt Technology Corporation

Expires: 07 Apr 2024

Storage: 2-8 °C after opening, DO NOT FREEZE

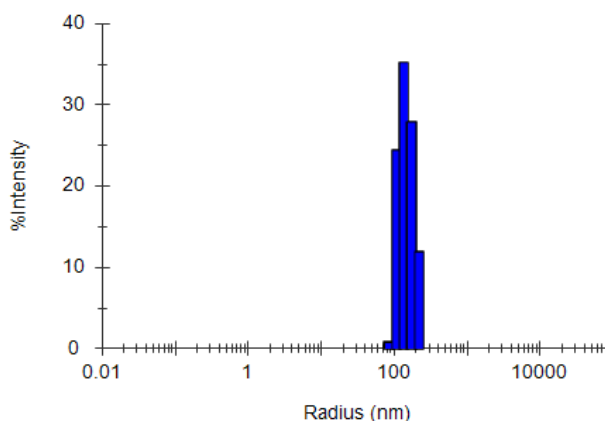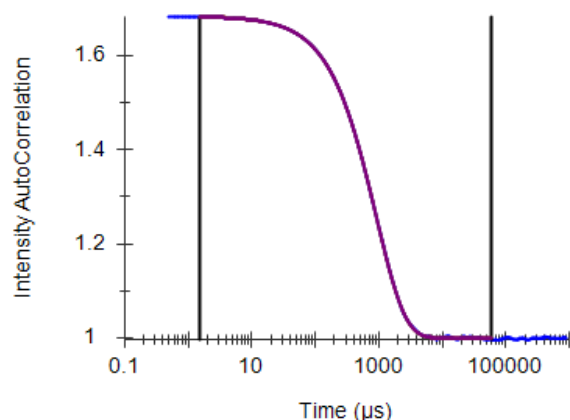

Standard characterization data by Wyatt DynaPro® dynamic light scattering instruments:

Sample was measured neat at 25 °C.

R_h (Cumulants) = (142 ± 3) nm

R_h (Regularization) = (142 ± 4) nm

Certification: Sophia Kenrick
Sophia Kenrick
Director of Analytical Sciences

Date: 07 Apr 2023